

Utah State University

DigitalCommons@USU

Reports

Utah Water Research Laboratory

January 1984

Use of the Hewlett-Packard 9810 Calculator System in Water Quality Analysis

Jerald S. Fifield

Follow this and additional works at: https://digitalcommons.usu.edu/water_rep



Part of the [Civil and Environmental Engineering Commons](#), and the [Water Resource Management Commons](#)

Recommended Citation

Fifield, Jerald S., "Use of the Hewlett-Packard 9810 Calculator System in Water Quality Analysis" (1984). *Reports*. Paper 493.

https://digitalcommons.usu.edu/water_rep/493

This Report is brought to you for free and open access by the Utah Water Research Laboratory at DigitalCommons@USU. It has been accepted for inclusion in Reports by an authorized administrator of DigitalCommons@USU. For more information, please contact digitalcommons@usu.edu.



USE OF THE HEWLETT-PACKARD 9810
CALCULATOR SYSTEM IN WATER QUALITY ANALYSIS

BY

JERALD S. FIFIELD

99886

USE OF THE HEWLETT-PACKARD 9810
CALCULATOR SYSTEM IN WATER QUALITY ANALYSIS

BY

JERALD S. FIFIELD

TABLE OF CONTENTS

	Page
Initilization Procedure Instructions	1
Plotter Board Instructions	4
Alkalinity, Calcium or Total Hardness	7
C.O.D.	10
Iron, Ammonia, Orthophosphate, or Nitrite Standardization Curve	14
Mean, S.D. and C.V. for NH_3 , Fe, N, or P	18
D.O. and/or B.O.D.	21
Graphing	27
Bibliography	35


Introduction

It is the purpose of this manual to illustrate the utilization of the Hewlett-Packard, Model 9810A calculator for analyzing water quality data. Familiarization of each program's capabilities is essential for successful application, thus the user should read over the section used before beginning. Each section is complete with instructions and illustrative examples.

INITIALIZATION PROCEDURE INSTRUCTIONS

INITIALIZATION PROCEDURE

Listed below are the keys which may be used for this section.

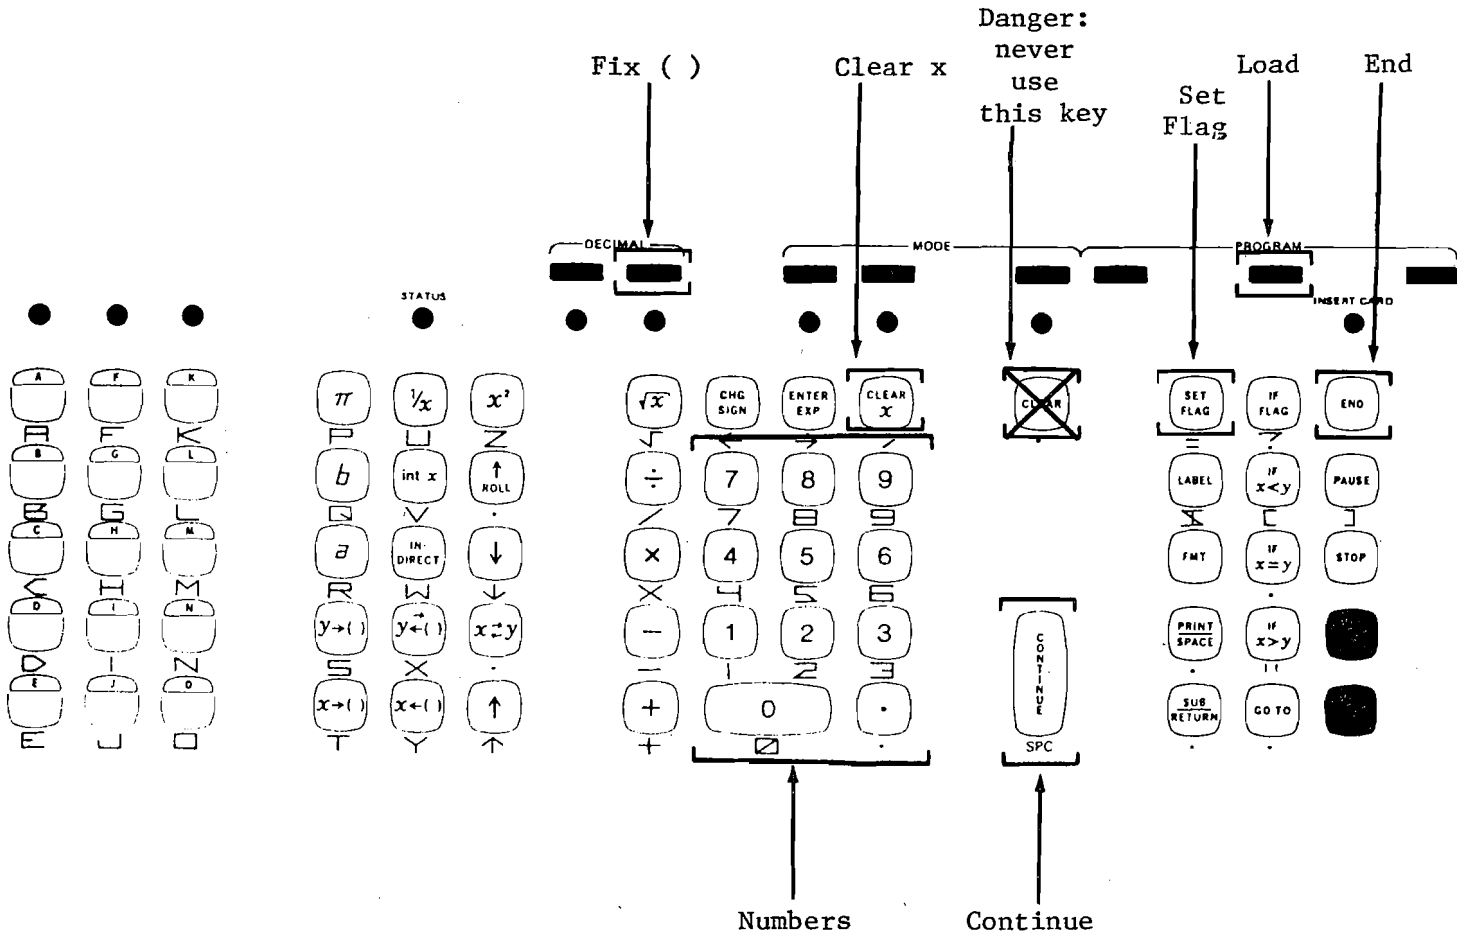

INITIALIZATION

3

1. Turn on computer.
2. Turn on cassette memory and insert tape.
3. Push END.
4. Insert magnetic card in the Reader, push LOAD and remove magnetic card.
5. Push END.
6. Push CONTINUE.
7. Enter one of the following numbers, then CONTINUE.

<u>Number</u>	<u>Program</u>
0	alkalinity
1	calcium
2	total hardness
3	C.O.D.
4	iron standard curve
6	ammonia standard curve
8	orthophosphate standard curve
10	nitrite standard curve
12	mean, S.D., and C.V. for NH ₃ , Fe, N, or P
14	D.O. and/or B.O.D.
16	graphs (includes linear regression)

8. Follow instructions printed by the computer and/or those stated in the manual.

PLOTTER BOARD INSTRUCTIONS

PLOTTER BOARD INSTRUCTIONS

INITIALIZATION


1. Push LINE ON. The button should stay down.
2. Push CHART HOLD. The button should stay down.
3. Push UPPER RIGHT.
4. Push CHART HOLD. The button should stay up.
5. Place your paper on the board. Remove the plastic tip from the pen and put it in the plotting position (i.e., the tip facing the paper).
6. Push CHART HOLD. The button should stay down.
7. Push LOWER LEFT. Adjust the pen to the desired position on the lower left section of your paper by manipulating the two knobs located at the immediate left of the LOWER LEFT button.
8. Push UPPER RIGHT. Adjust the pen to the desired position on the upper right section of your paper by manipulating the two knobs located at the immediate right of the UPPER RIGHT button.
9. Push LOWER LEFT to check the position of the pen. Repeat steps 7 and 8 until you are satisfied with the position of the pen.
10. Continue with the desired program.

TERMINATION

1. Push UPPER RIGHT.
2. Replace the plastic cap on the pen. Remove the pen from the plotting position (i.e., the tip nob facing the paper).
3. Push CHART HOLD. The button should stay up.
4. Remove your graph.
5. If another graph is to be developed, proceed to step 5 of the initialization procedure above.
6. If no more graphs are to be drawn, push LINE ON. The button should stay up.

<u>Number</u>	<u>Program</u>
0	alkalinity
1	calcium
2	total hardness
3	C.O.D.
4	iron standardization curve
6	ammonia standardization curve
8	orthophosphate standardization curve
10	nitrite standardization curve
12	mean, S.D. and C.V. for NH ₃ , Fe, N, or P
14	D.O. and/or B.O.D.

Listed below are the keys which may be used for the above programs.

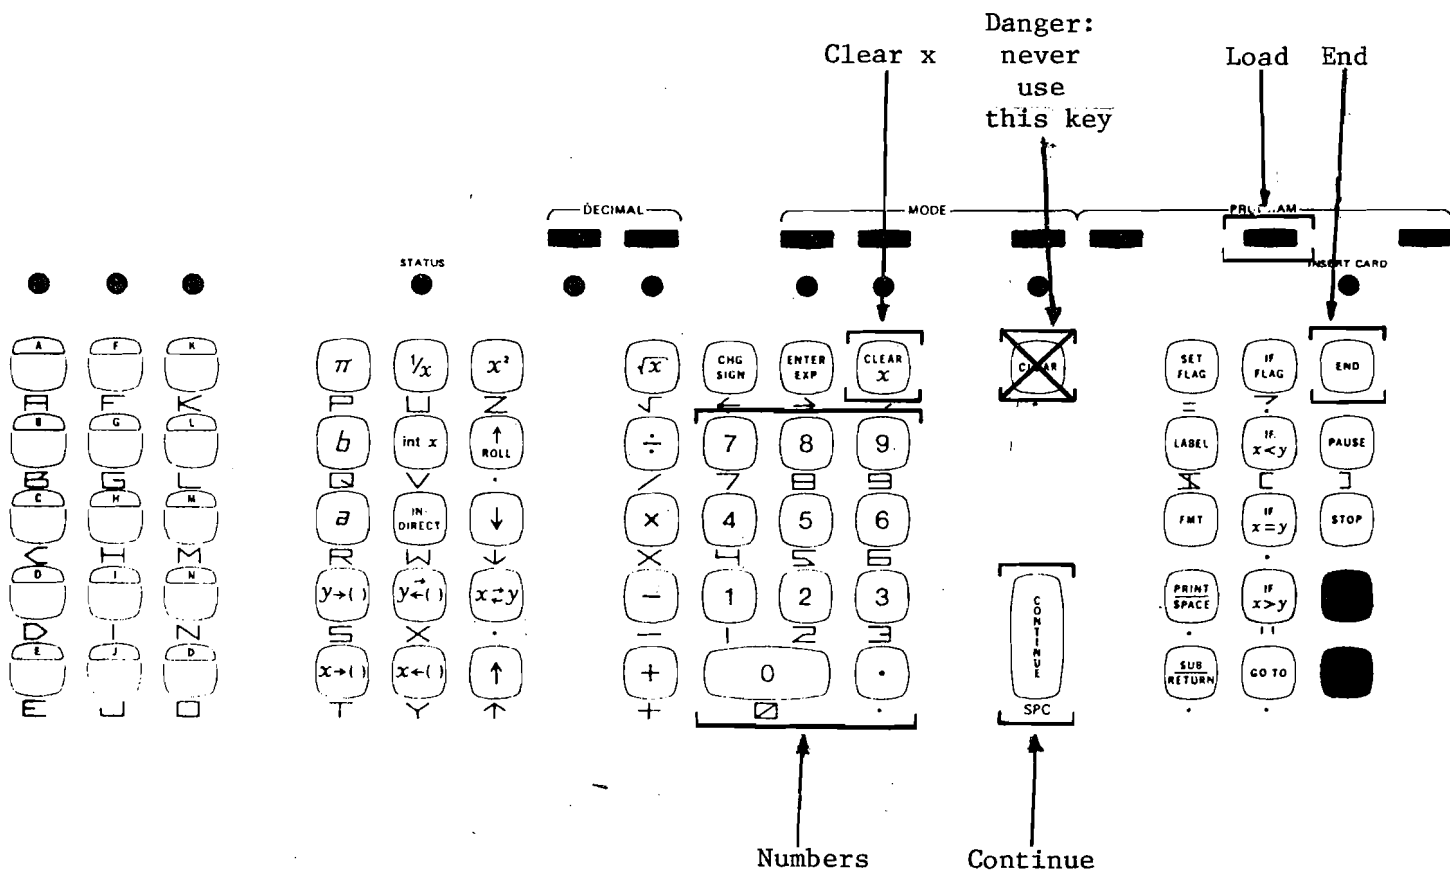

INSTRUCTIONS

NUMBERPROGRAM

0

ALKALINITY

1

CALCIUM

2

TOTAL HARDNESS

1. Follow initialization procedure (if not done already).
2. NOTE: If an incorrect entry occurs, and CONTINUE has not been executed, push CLEAR X and enter correct value. If CONTINUE was executed and a mistake discovered, start anew by pushing END, then CONTINUE.

TOTAL HARDNESS	} Title of program.
PUSH "SET FLAG" IF STANDARD HAS BEEN CALIBRATED STANDARD CALIBRATION	} For an initial run, push CONTINUE. If the stan- dard has been calibrated, push SET FLAG, then CONTINUE and go to Step 3.
ENTER NORMALITY 0.02500*	} Information required to calibrate normality of the standard. Enter what is requested, then push CONTINUE. The numbers indicate what was entered.
VOLUME OF STANDARD USED (IN MLS) 10.00000*	
ENTER FOL (MLS) OF TITRANT USED ENTRY 1.00000 10.20000	} Amount of titrant used per sample in calibrating the standard. Enter a value, then CONTINUE. Repeat until all data has been entered (minimum entry is 2). The first number is a counter and the second indicates what was entered.
ENTRY 2.00000 10.25000	
ENTRY 3.00000 11.00000	
ENTRY 4.00000	} When all data has been entered, push SET FLAG, then CONTINUE.
NORMALITY MEAN 0.02385	} Statistics on the actual normality of your standard.
S.D. 0.00102	
C.V.(%) 4.27483	

3. Once the standard has been calibrated, the following will be executed:

MLS OF SAMPLE=?	50.00000*	}	Enter the volume of your sample, then push CONTINUE. The number indicates what was entered.
ENTER VOL (MLS) OF TITRANT USED ENTRY	1.00000 5.30000		
ENTRY	2.00000 5.60000	}	Amount of titrant used per sample. Enter a value, then push CONTINUE. Repeat until all data has been entered (minimum entries is 2). The first number is a counter and the second indicates what was entered.
ENTRY	3.00000 5.50000		
ENTRY	4.00000	}	When all data has been entered, push SET FLAG, then CONTINUE.
TOTAL HARDNESS (MG/L AS CAC03) MEAN	260.73132		
S.D.	7.28549	}	Statistics for your desired program. Push PAPER to remove your copy.
C.V. (%)	2.79425		

4. If the same program is to be run again, push END, then CONTINUE.
5. If another program is desired, follow the procedure outlined in that section.
6. If no other program is to be run, turn off the computer and cassette memory.

INSTRUCTION

NUMBER

3

PROGRAM

C.O.D.

1. Follow initialization procedure (if not done already).
2. NOTE: If an incorrect entry occurs, and CONTINUE has not been executed, push CLEAR X and enter correct value. If CONTINUE was executed and a mistake discovered, start anew by pushing END, then CONTINUE.

C.O.D.	} Title of program
PUSH "SET FLAG" IF STANDARD HAS BEEN CALIBRATED	} For an initial run, push CONTINUE. If the standard has been calibrated, push SET FLAG, then CONTINUE and go to step 3.
NORMALITY=? 0.25000*	} Information required to calibrate normality of the standard. Enter what is requested, then push CONTINUE. The numbers indicate what was entered.
VOLUME OF STANDARD USED (IN MLS) 10.00000*	
ENTER VOL (MLS) OF TITRANT USED ENTRY 1.00000 10.10000	} Amount of titrant used per sample in calibrating the standard. Enter a value, then CONTINUE. Repeat until all data has been entered (minimum entries is 2). The first number is a counter and the second indicates what was entered.
ENTRY 2.00000 10.00000	
ENTRY 3.00000 10.20000	} When all data has been entered, push SET FLAG, then CONTINUE.
ENTRY 4.00000	
NORMALITY MEAN 0.24752	} Statistics on the actual normality of your standard.
S.D. 0.00245	
C.V.(%) 0.99010	

3. Once the computer has calibrated the standard, the following steps are executed:

MLS OF SAMPLE=? 20.00000	} Enter the volume of your sample, then push CONTINUE. The number indicates the entry.
-----------------------------	-------------------------------------------------------------------------------------------

BLANK		
ENTER VOL (MLS)		
OF TITRANT USED		
ENTRY	1.000000	Amount of titrant used for the <u>blanks</u> . Enter a value, then CONTINUE. Repeat until all data has been entered (minimum entry = 2). The first number is a counter and the second is the entry.
	25.300000	
ENTRY	2.000000	When all data has been entered, push SET FLAG, then CONTINUE.
	24.700000	
ENTRY	3.000000	Statistics for your blank.
MEAN	25.000000	
S.D.	0.42426	
C.V. (%)	1.69706	
SAMPLE		
ENTER VOL (MLS)		
OF TITRANT USED		
ENTRY	1.000000	Amount of titrant used for the <u>samples</u> . Enter a value, then CONTINUE. Repeat until all data has been entered (minimum entry = 2). The first number is a counter and the second is the entry.
	22.000000	
ENTRY	2.000000	When all data has been entered, push SET FLAG, then CONTINUE.
	22.100000	
ENTRY	3.000000	Statistics for your sample.
	20.800000	
ENTRY	4.000000	C.O.D. of your sample. Push PAPER to remove your copy.
	21.300000	
ENTRY	5.000000	
	21.400000	
ENTRY	6.000000	
MEAN	21.520000	
S.D.	0.53572	
C.V. (%)	2.48942	
C.O.D. (MG/L)	344.55446	

4. If the program is to be run again, push END, then CONTINUE.
5. If another program is desired, follow the procedure outlined in that section.
6. If no other program is to be run, turn off the computer and cassette memory.

INSTRUCTIONS

<u>NUMBER</u>	<u>PROGRAM</u>
4	IRON STANDARDIZATION CURVE
6	AMMONIA STANDARDIZATION CURVE
8	ORTHOPHOSPHATE STANDARDIZATION CURVE
10	NITRITE STANDARDIZATION CURVE

1. Follow the procedure for setting up your graph on the plotter.
2. Follow initialization procedure (if not already done).
3. Note: If an incorrect entry occurs, and CONTINUE has not been executed, push CLEAR X and enter correct value. If CONTINUE was executed and a mistake discovered, start anew by pushing END, then CONTINUE.

NITRITE		} Title of program.
MAX ABSORPTION=?		
	0.600*	} Enter the largest value you want for the absorbance axis, then CONTINUE. The number indicates what was entered.
WAVELENGTH=?		
	543.000	} General information for your graph. Enter what is requested, then CONTINUE.
CELL LENGTH=?		
	1.000	} Coordinates to be entered for plotting your points: X=Concentration Y=Absorbance
CELL UNITS		
(1 = IN. 2 CM)		} At least 3 points are needed. Enter X, then CONTINUE. Enter Y, then CONTINUE. Arrange your data such that X is in <u>ascending</u> order.
X=?		
	35.000*	} When all points have been plotted, push SET FLAG, then CONTINUE. The best straight line will be drawn and an equation, with R^2 , written on your graph. (See page 17.)
Y=?		
	0.118*	}
X=?		
	70.000	}
Y=?		
	0.260*	}
X=?		
	105.000	}
Y=?		
	0.355*	}
X=?		
	140.000	}
Y=?		
	0.510*	}
X=?		

4. The following will illustrate how concentrations can be found if you know absorbance.

EQUATION	
Y=?	
X=	0.15200*
Y=?	43.78442
X=	0.30000*
Y=?	84.53973
X=	0.52300*
Y=?	145.94807

Enter the absorbance (i.e., Y) of your sample, then CONTINUE. The X represents concentrations in mg/l.

5. Push the HOLD button (it should stay up). Remove your graph.
6. If this, or any other program is to be run again, follow the procedure for that section.
7. If no other program is to be run, turn off the computer, cassette memory, and plotter board. Be sure the plastic lid is on the tip of the pen.


NITRITE

WAVELENGTH = 543. NM

CELL LENGTH = 1. CM

$Y = 0.00353 X + (-0.00700)$

R-SQ = 0.99245

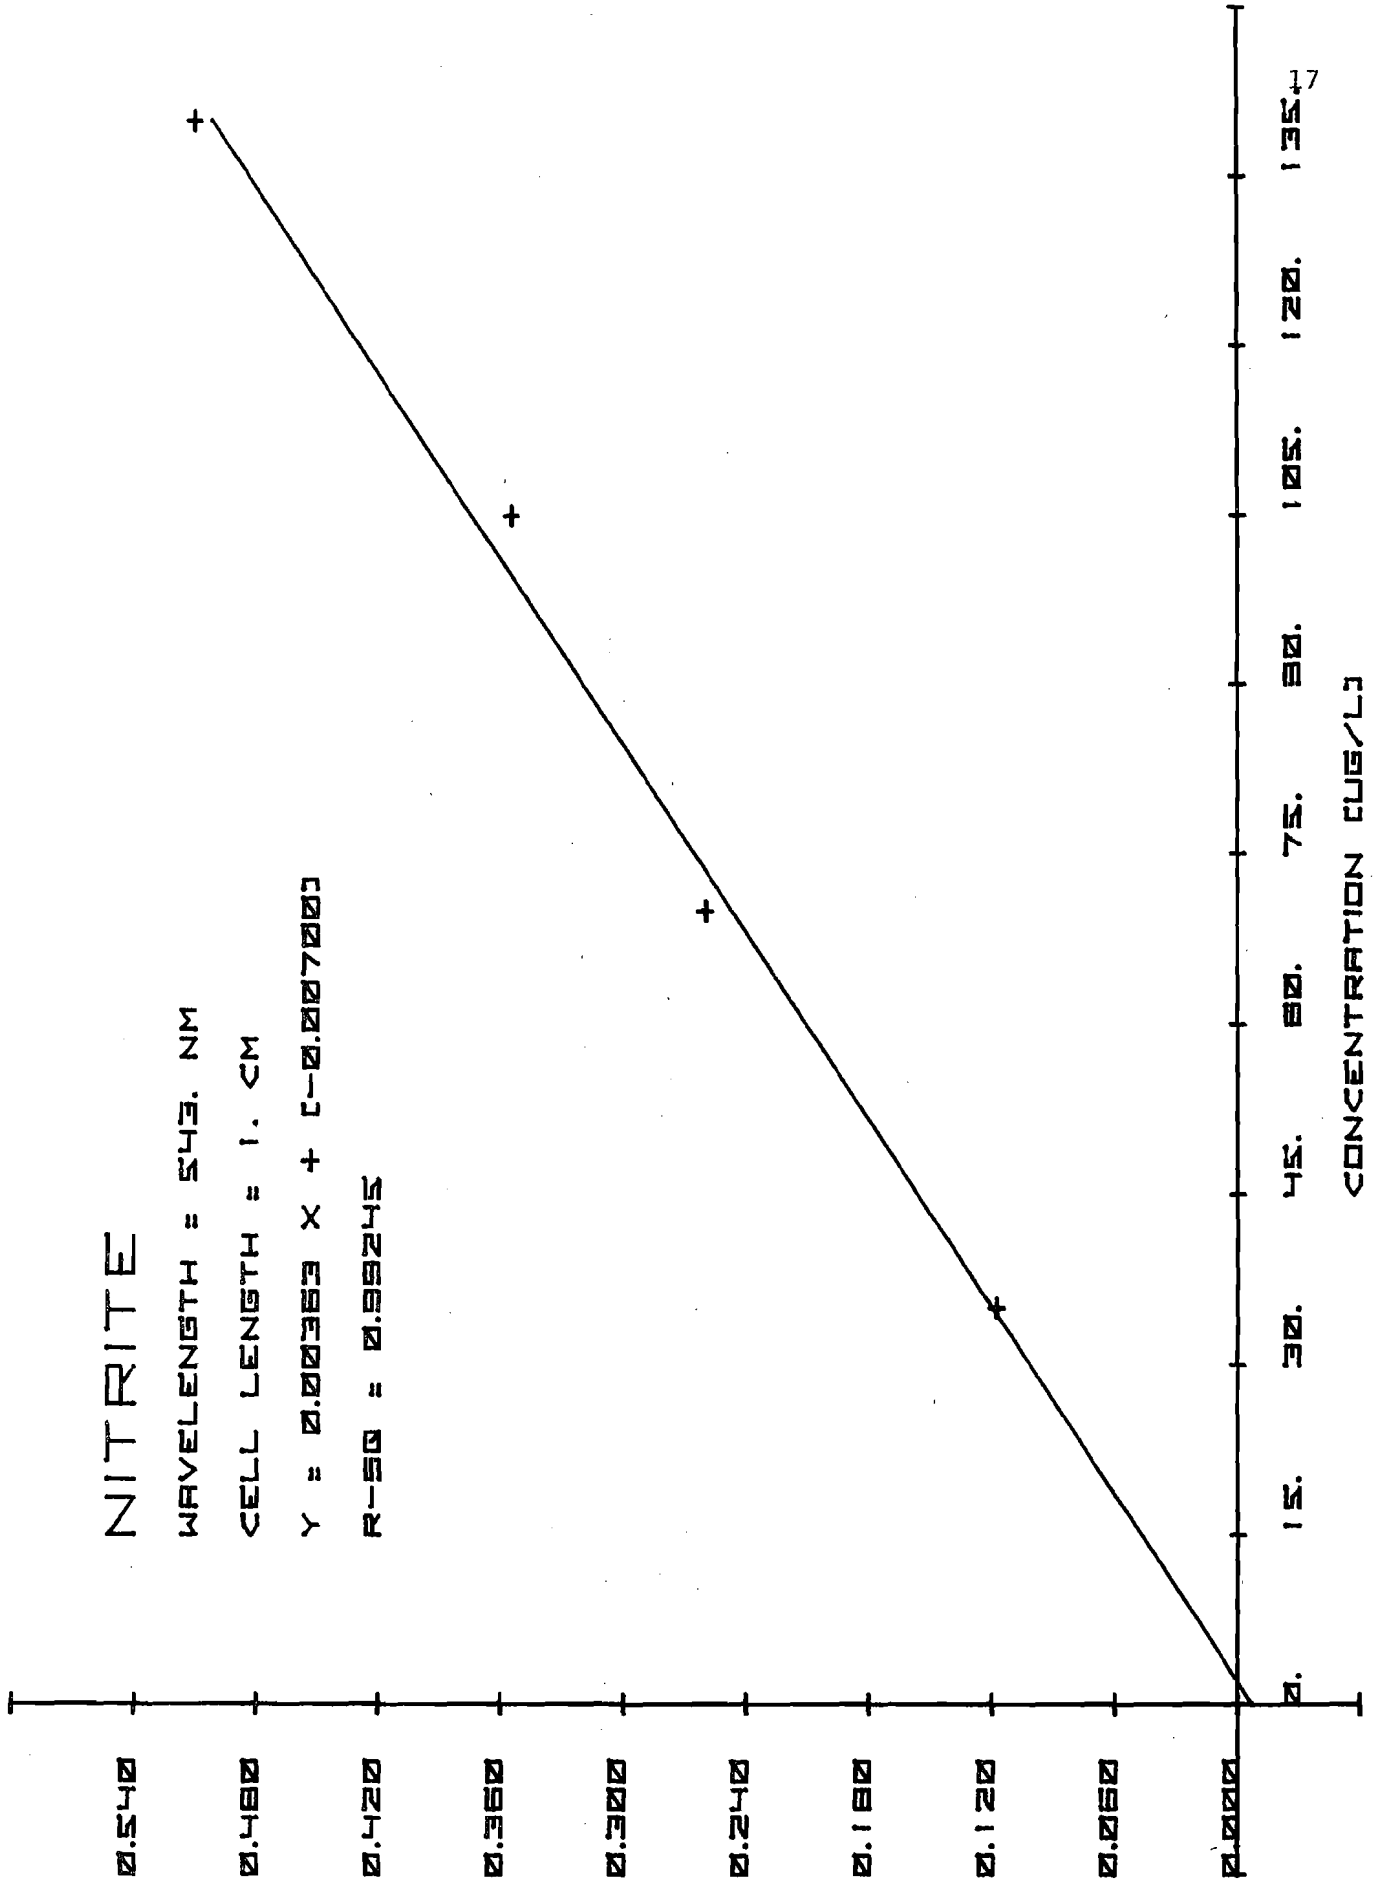

INSTRUCTIONS

NUMBERPROGRAM

12

MEAN, S.D., AND C.V. FOR NH₃,
FE, N, OR P

1. Follow initialization procedure (if not already done).
2. NOTE: If an incorrect entry occurs, and CONTINUE has not been executed, push CLEAR X and enter correct value. If CONTINUE was executed and a mistake discovered, start anew by pushing END, then CONTINUE.

MEAN, S.D., AND C.V. FOR AMMONIA IRON, NITRITE OR ORTHOPHOSPHATE	} Title of program
ENTER ABSORBANCE ENTRY	} Absorbance readings of your sample. Enter a value then CONTINUE. Repeat until all data has been entered (minimum entries is 2). The first number is a counter and the second indicates what was entered.
1.00000 0.14000	
ENTRY	
2.00000 0.14500	
ENTRY	
3.00000 0.14500	
ENTRY	} When all data has been entered, push SET FLAG, then CONTINUE.
4.00000 0.14300	
ENTRY	
5.00000 0.14900	} Statistics on the absorbance of your samples.
ENTRY	
6.00000 0.13300	
ENTRY	} Option to allow the user to go to a standard curve without having to go to the initialization procedure.
7.00000	
MEAN	
0.14250	
S.D.	
0.00550	
C.V. (%)	
3.86284	
ENTER VALUE IF GRAPHING STANDARD CURVE	
4 = FE	
6 = NH3	
8 = P	
10 = N	

3. If the program is to be run again, push END, then CONTINUE.

4. If another program is desired, follow the procedure outlined in that section.
5. If no other program is to be run, turn off the computer and cassette memory.

INSTRUCTIONS

NUMBERPROGRAM

14

D.O. AND/OR B.O.D.

1. Follow initialization procedure (if not already done.)
2. NOTE: If an incorrect entry occurs, and CONTINUE has not been executed, push CLEAR X and enter correct value. If CONTINUE was executed and a mistake discovered, start anew by pushing END, then CONTINUE.

DO AND/OR BOD	} Title of program
DO ONLY? (1=YES 2=NO)	} Choose between D.O. or B.O.D. The number indicates what choice was made.
1.000000*	
PUSH "SET FLAG" IF STANDARD HAS BEEN CALIBRATED STANDARD CALIBRATION	} For an initial run, push CONTINUE. If the standard has been calibrated, push SET FLAG, then CONTINUE and go to D.O. or B.O.D. instructions.
ENTER NORMALITY 0.02500*	} Information required to calibrate normality of the standard. Enter what is required, then push CONTINUE. The numbers indicate what was entered.
MLS OF STANDARD 20.00000*	
ENTER VOL (MLS) OF TITRANT USED ENTRY 1.000000 20.200000	} Amounts of titrant used per sample in calibrating the standard. Enter a value then CONTINUE. Repeat until all data has been entered (minimum entry is 2). The first number is a counter and the second indicates what was entered.
ENTRY 2.000000 20.200000	
ENTRY 3.000000 20.200000	
ENTRY 4.000000	} When all data has been entered, push SET FLAG, then CONTINUE.
NORMALITY MEAN 0.02475	} Statistics on the actual normality of your standard.
S.D. 0.000000	
C.V. (%) 0.000000	

D.O. Instructions

1 ML OF .025 N NA2S2O3 EQUALS 0.99010 MG OF O2/L AS DO D.O.	} Equivalence of $\text{Na}_2\text{S}_2\text{O}_3$ to milligrams/liter of O_2 .
SAMPLE 1.000000	} Identifies what sample is being analyzed for D.O.
ENTER VOL (MLS) OF TITRANT USED ENTRY 1.000000 3.000000	} Amount of titrant used. Enter a value, then CONTINUE. Repeat until all data has been entered (minimum entry is 2). The first number is a counter and the second is the entry.
ENTRY 2.000000 2.900000	
ENTRY 3.000000 3.100000	} When all data has been entered, push SET FLAG, then CONTINUE.
ENTRY 4.000000	
MEAN 2.97030	} Statistics of D.O. for your sample. The mean and S.D. are final D.O. values (in mg/l of O_2).
S.D. 0.09901	
C.V. (%) 3.33333	
SAMPLE 2.000000	} Identifies the next sample being analyzed.
ENTER VOL (MLS) OF TITRANT USED ENTRY 1.000000 0.700000	} Amount of titrant used. Enter a value, then CONTINUE. Repeat until all data has been entered (minimum entry is 2). The first number is a counter and the second is the entry.
ENTRY 2.000000 8.500000	
ENTRY 3.000000 8.400000	} When all data has been entered, push SET FLAG, then CONTINUE.
ENTRY 4.000000	
MEAN 8.44884	} Statistics of D.O. for your sample. The mean and S.D. are final D.O. values (in mg/l of O_2).
S.D. 0.15124	
C.V. (%) 1.79007	

3. Continue in a similar manner until all your samples have been analyzed for D.O.

B.O.D. Instructions

B.O.D.	} Title of program
SET FLAG WHEN SAMPLE CALCULA- TIONS ARE COM- PLETED	} If D.O. samples are to be calculated push CONTINUE
DO SAMPLE 1.000000	} Titrant entries to calculate the D.O. of your sample. Enter value, then CONTINUE (a minimum of 2 entries is required). The first number is a counter and the second represents what was entered
ENTER VOL (MLS) OF TITRANT USED ENTRY 1.000000 7.510000	
ENTRY 2.000000 7.610000	
ENTRY 3.000000 7.510000	
ENTRY 4.000000	
MEAN 7.46865	
S.D. 0.05716	} When all data has been entered, push SET FLAG, then CONTINUE
C.V. (%) 0.76538	} Statistics of D.O. for your sample. The mean and S.D. are final D.O. values (in mg/l of O ₂).
DO SAMPLE 2.000000	} If all samples have been calculated for D.O. then push SET FLAG, and CONTINUE. Otherwise, push CONTINUE.
DECIMAL FRACTION OF SAMPLE=? 0.050000	} Enter the fraction of your sample used, then CONTINUE. The number represents what was entered.
BLANK 1=? 7.75000*	} Enter the initial blank D.O. value, then CONTINUE.
BLANK 2=? 7.10000*	} Enter the second blank D.O. value, then CONTINUE.
D.O. 1=? 7.47000*	} Enter the initial sample D.O. value, then CONTINUE.
D.O. 2=? 6.49000*	} Enter the second D.O. value, then CONTINUE.
MG BOD/L EQUALS 6.60000	} The BOD for that particular day being analyzed.
DECIMAL FRACTION OF SAMPLE=?	} Repeat the above until all days have been completed.

4. Push PAPER to remove your copy.
5. If this, or another, program is to be run again, follow the procedure outlined in that section.
6. If no other program is to be run, turn off the computer and cassette tape drive.

INSTRUCTIONS

NUMBER

16

PROGRAMGRAPHING (INCLUDES LINEAR
REGRESSIONS)

1. Follow initialization procedure (if not already done).

INITIALIZATION ENTER PROGRAM NUMBER PUSH FIX(), THEN ENTER THE NUMBER OF DIGITS YOU WANT AFTER THE DECIMAL POINT FOR THE AXIS FINALLY, PUSH CONTINUE <div style="text-align: right;">16.</div>	} Enter 16, then CONTINUE. } This allows you to select the number of digits after the decimal point desired if it is decided to allow the computer to draw and label each axis. } Program number chosen.
-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------	--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

2. NOTE: If an incorrect entry occurs, and CONTINUE has not been executed, push CLEAR X and enter correct value. If CONTINUE was executed and a mistake discovered, start anew by pushing END then CONTINUE.
3. Follow Plotter Instructions

GRAPHING X-MAX =? 150. X-MIN =? 0. Y-MAX =? 150. Y-MIN =? 0. ARE YOU PLOTTING ON GRAPH PAPER? (0=NO 1=YES)	} Title of program. } Maximum and minimum coordinates of your graph. Choose numbers which will include your values to be plotted adequately. } If 0 is entered, a graph will be drawn with the ordinates and abscissa each divided into ten equal parts. After the graph is developed, follow the linear regression or non-linear regression instructions.
---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------	--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Linear Regression Instructions

```

LINEAR REG?
(0 = NO  1 = YES)
X=?
      10.0000
Y=?
      25.0000*
X=?
      45.0000
Y=?
      45.0000*
X=?
      90.0000
Y=?
      125.0000*
X=?

```

} Enter 1, then CONTINUE.

} Once the linear regression option has been selected, enter the coordinates as requested, then CONTINUE. These points will be plotted on your graph.

} When all data has been entered, push SET FLAG, then CONTINUE. On your graph, the best straight line will be drawn along with the equation and R^2 value written. (See the graph on page 32.)

```

LINEAR REG. WAS
EXECUTED

```

```

GENERAL EQUATION
IS Y = MX + B

```

```

DO YOU WANT TO
ENTER X AND
SOLVE FOR Y?
(0=NO, 1=YES)

```

```

Y=?
      90.000000*
X=
      67.94723
Y=?
      33.500000*
X=
      23.61995
Y=?

```

} This allows you to use the linear regression equation developed to solve for the dependent variable (i.e. Y) or independent variable (i.e. X). Enter 0 or 1, then CONTINUE.

} Example of solving for the independent variable (i.e. X) when Y is known. Enter value of Y, then CONTINUE (Repeat as often as desired).


X=?	150.00000*
Y=	194.58528
X=?	72.60000*
Y=	95.93047
X=?	

Example of solving for the dependent variable (i.e. Y) when X is known. Enter value of X, then CONTINUE (Repeat as often as desired).

4. Remove graph from plotter.
5. To run this or any other program, follow the procedure of that section.
6. If no other program is to be run, turn off the computer, cassette memory and plotter board (the ON button should be up).
7. Be sure the plastic lid is on the tip of the ink pen.

$$Y = 1.27461 X + 63.383763$$

$$R^2 = 0.83320$$

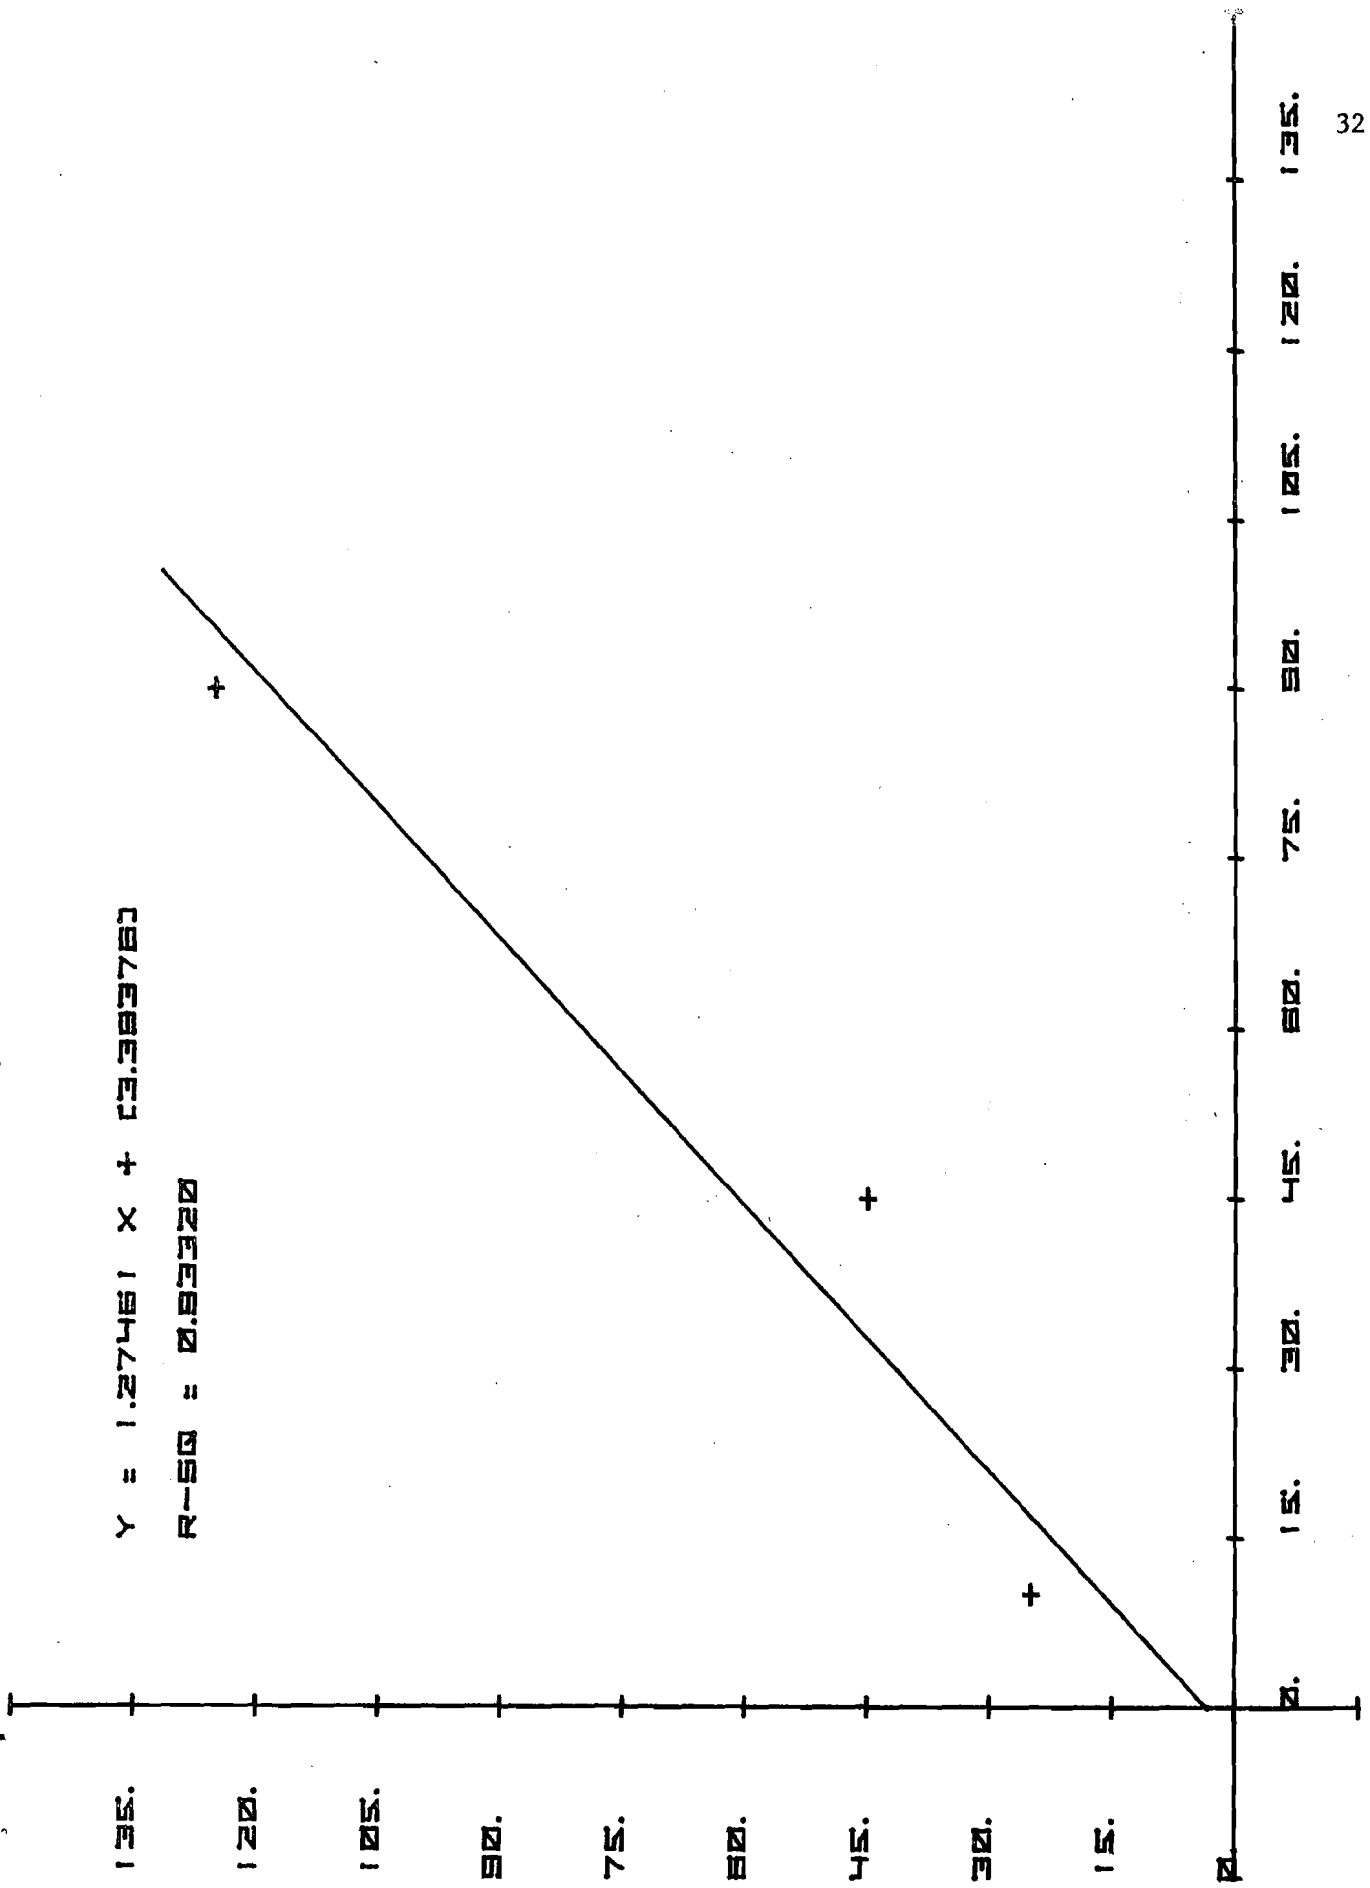

Non Linear Regression Instructions

<pre> GRAPHING X-MAX =? 200. X-MIN =? 0. Y-MAX =? 150. Y-MIN =? 0. ARE YOU PLOTTING ON GRAPH PAPER? (0 = NO 1 = YES) LINEAR REG? (0 = NO 1 = YES) </pre>	} Title of program. } Maximum and minimum coordinates of your graph. } See, the linear regression instructions. } See the linear regression instructions } Enter 0, then CONTINUE.
----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------	------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

8. NOTE: As the program is written, each point will be marked with a "+"
This may be altered by the following steps:

- 1) push GO TO 0462
- 2) push PRGM
- 3) push:
 - a) FMT
 - b) 1
 - c) FMT
 - d) any number or symbol desired
 - e) FMT
- 4) push RUN
- 5) push 0.1, then FMT 11
- 6) push END, then CONTINUE

This must be executed before a decision on connection points is made.
This allows more than one curve to be put on a single graph.

```


CONNECT POINTS?
(0=NO, 1=YES)
X=?
      20.0000
Y=?
      10.0000*
X=?
      30.0000
Y=?
      32.5000*
X=?
      60.0000
Y=?
      65.0000*
X=?
     100.0000
Y=?
      98.0000*
X=?
     150.0000
Y=?
     120.0000*
X=?
     180.0000
Y=?
     130.0000*
X=?

```

This allows the option of connection each point with a straight line. Enter your choice, then CONTINUE

Enter your value for X, then CONTINUE. Enter your value for Y, then CONTINUE. Repeat the above until all data has been plotted.

9. If another curve is to be plotted on the same graph, go to step 8.
10. Remove your graph (see plotting instructions).
11. If no other program is to be run, turn off the computer, cassette memory and plotter board (the ON button should be up).
12. If this, or any other program is to be run, the initialization procedure for that section must be followed.

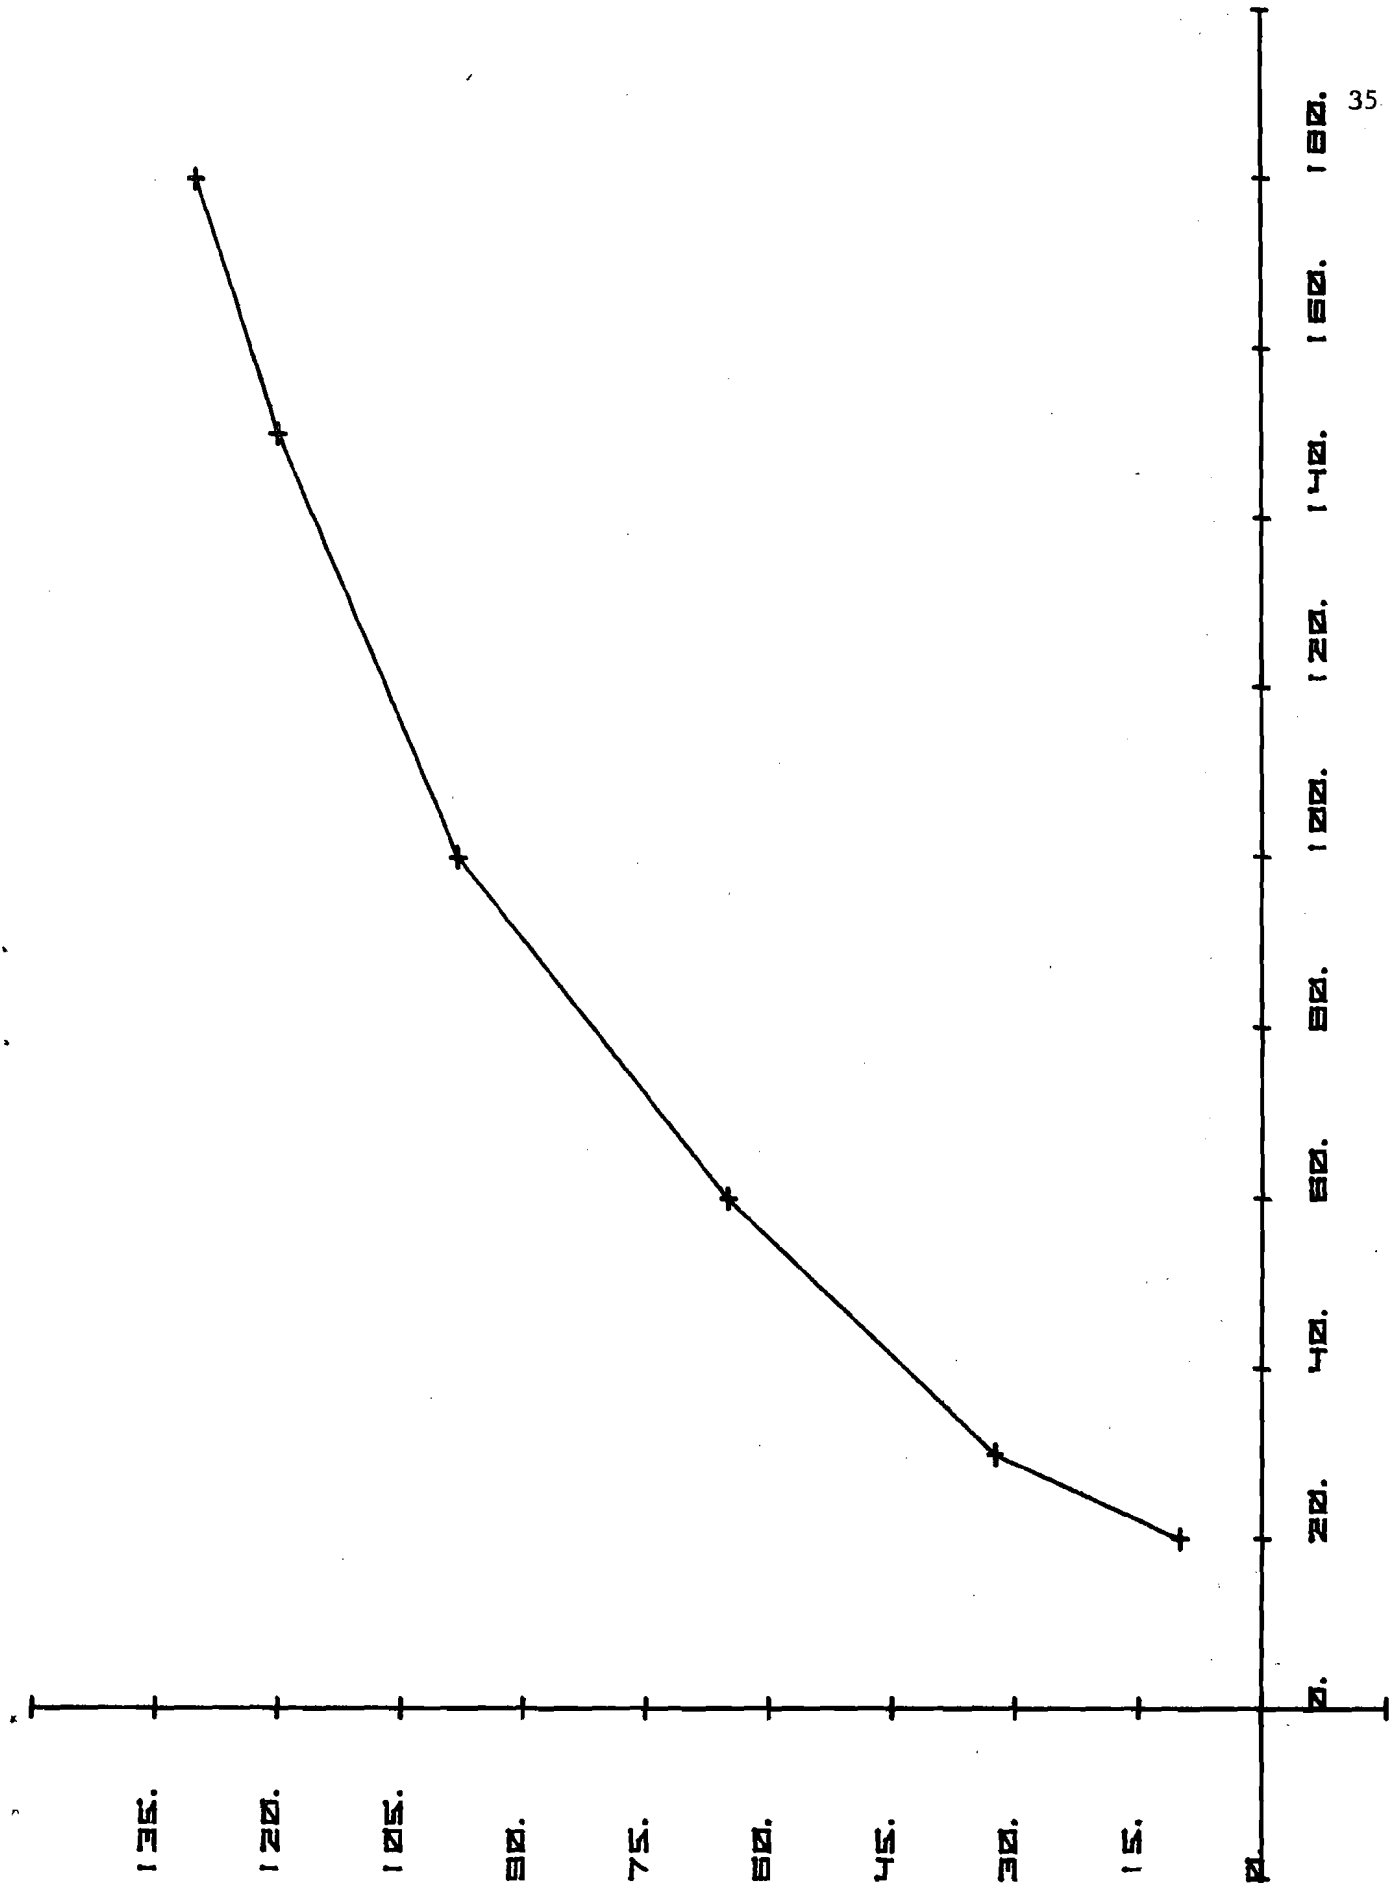

BIBLIOGRAPHY

Cowan, Pete and Don Porcella (eds.) 1975. Water Quality Analysis Laboratory Procedures Syllabus. 94 pages.

Hewlett-Packard Company. 1971. Hewlett-Packard 9810A Calculator Operating and Programming Manual. 151 pages.