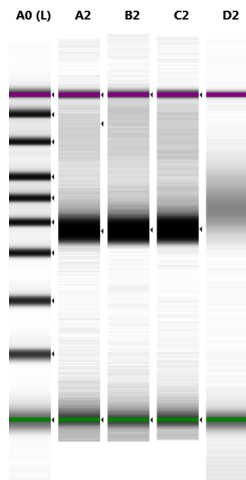



Filename: 2019-02-14-01 Walton Lau.HSD1000**Gel Image**

Default image (Contrast 100%), Image is Scaled to view larger Molecular Weight range

Sample Info

Well	Conc. [pg/ul]	Sample Description	Alert	Observations
A0	2350	Electronic Ladder		Ladder
A2	1470	Walton BP01		
B2	1700	Walton BP02		
C2	1660	Walton BP03		
D2	758	Lau WT2		

A0: Electronic Ladder

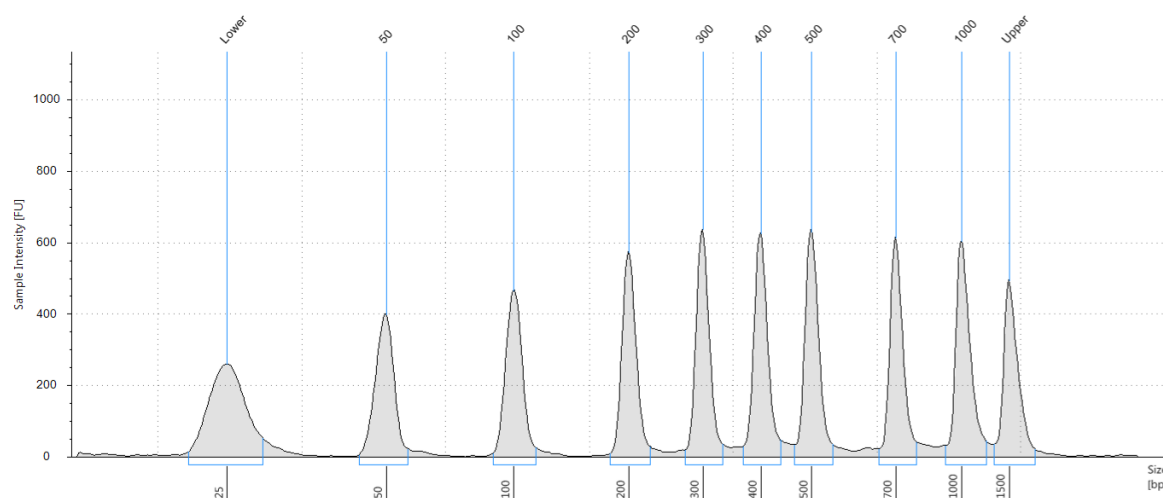


Sample Table

Well	Conc. [pg/ul]	Sample Description	Alert	Observations
A0	2350	Electronic Ladder		Ladder

Peak Table

Size [bp]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	340	-	20900	-		Lower Marker
50	265	-	8160	11.28		
100	278	-	4270	11.82		
200	290	-	2230	12.32		
300	304	-	1560	12.95		
400	306	-	1180	13.00		
500	312	-	961	13.29		
700	286	-	629	12.19		
1000	309	-	476	13.15		
1500	250	250	256	-		Upper Marker

A2: Walton BP01

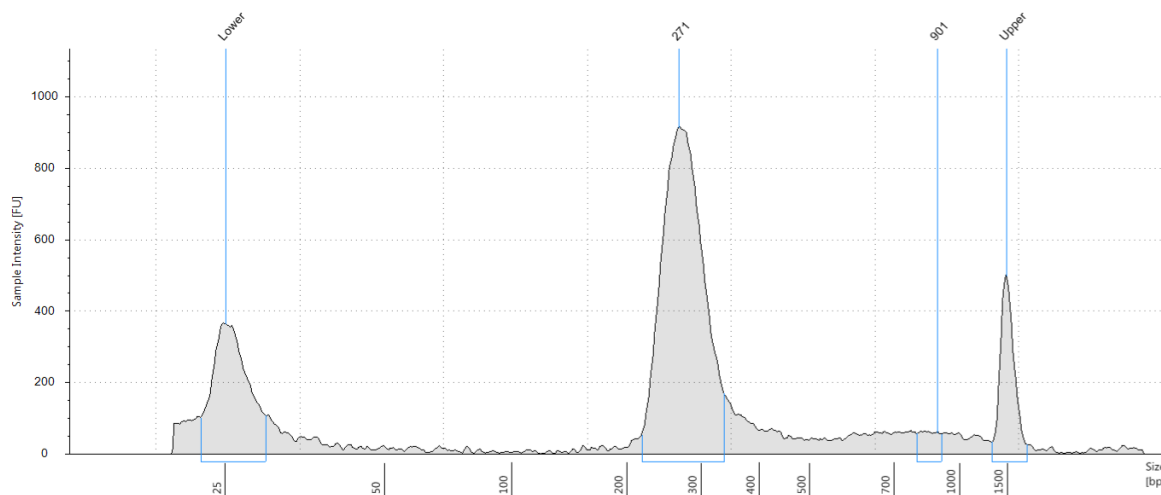


Sample Table

Well	Conc. [pg/ul]	Sample Description	Alert	Observations
A2	1470	Walton BP01		

Peak Table

Size [bp]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	485	-	29800	-		Lower Marker
271	1420	-	8090	96.87		
901	46.0	-	78.6	3.13		
1500	250	250	256	-		Upper Marker

B2: Walton BP02

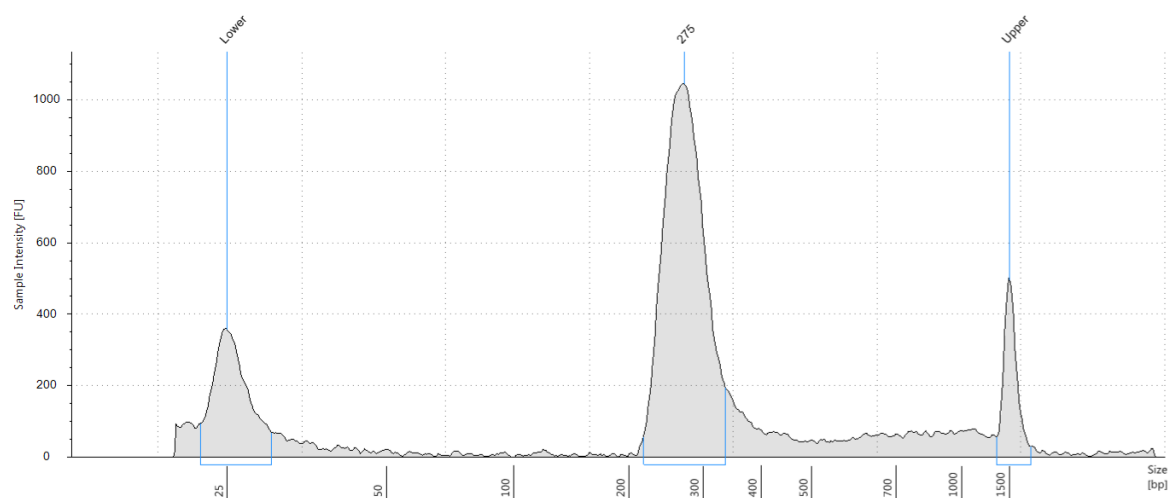


Sample Table

Well	Conc. [pg/ul]	Sample Description	Alert	Observations
B2	1700	Walton BP02		

Peak Table

Size [bp]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	487	-	30000	-		Lower Marker
275	1700	-	9550	100.00		
1500	250	250	256	-		Upper Marker

C2: Walton BP03

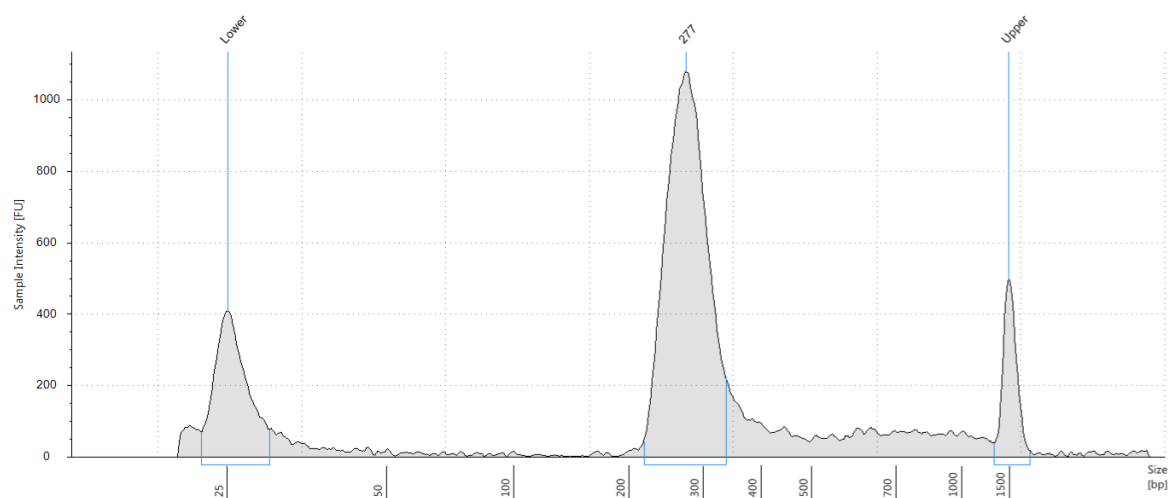

Sample Table

Well	Conc. [pg/ul]	Sample Description	Alert	Observations
C2	1660	Walton BP03		

Peak Table

Size [bp]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	483	-	29700	-		Lower Marker
277	1660	-	9200	100.00		
1500	250	250	256	-		Upper Marker